



Copy of New B-3 V-5 R-3 Y-5 UV-3

| | | | |
|-------------------|-----------|--------------|----------------------|
| Cytometer: | FACSriaII | User: | FHCRC |
| Cytometer Name: | FACSriaII | Institution: | N/A |
| Serial Number: | P96500035 | Software: | BD FACSDiva 8.0.1 |
| Input Device: | Manual | Date: | 3/23/2017 2:57:02 PM |
| Sheath Pressure: | 70.00 | | |
| Nozzle Size: | 70 | | |
| Window Extension: | 2.00 | | |


Red Laser (640nm)

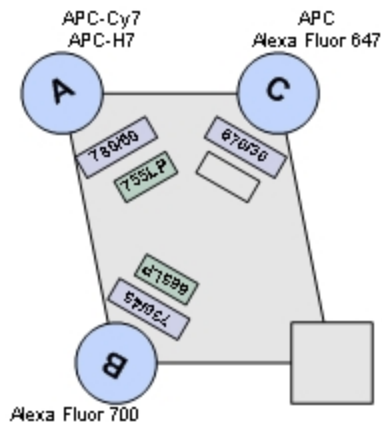


Blue Laser (488nm) FSC

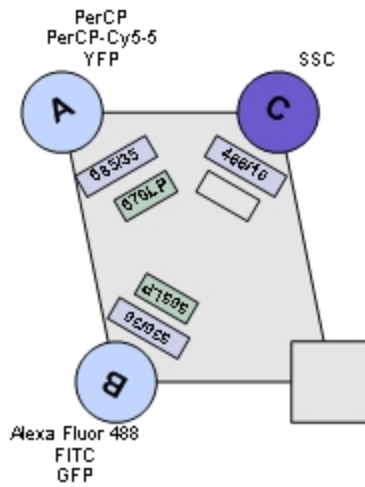


Yellow Green Laser
(561nm)

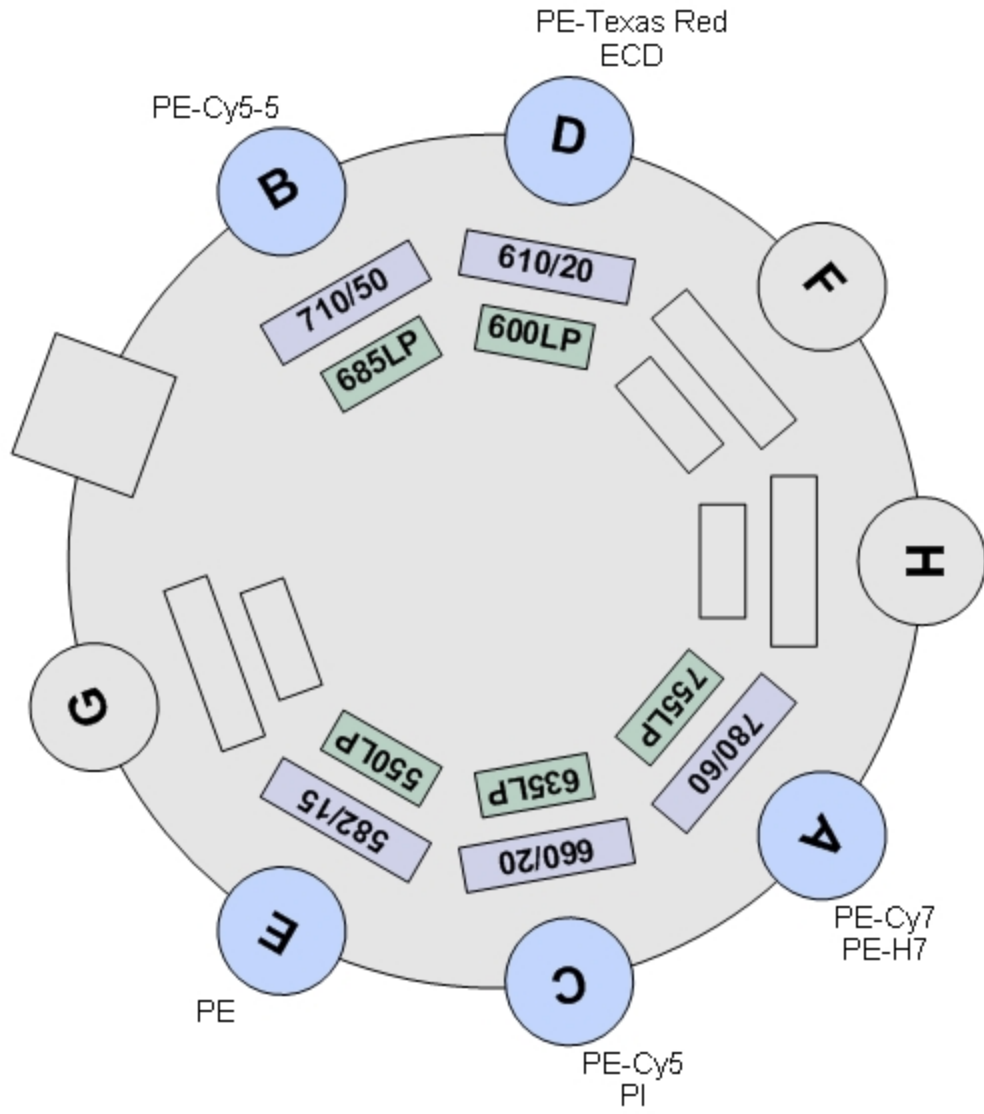

Violet Laser
(405nm)

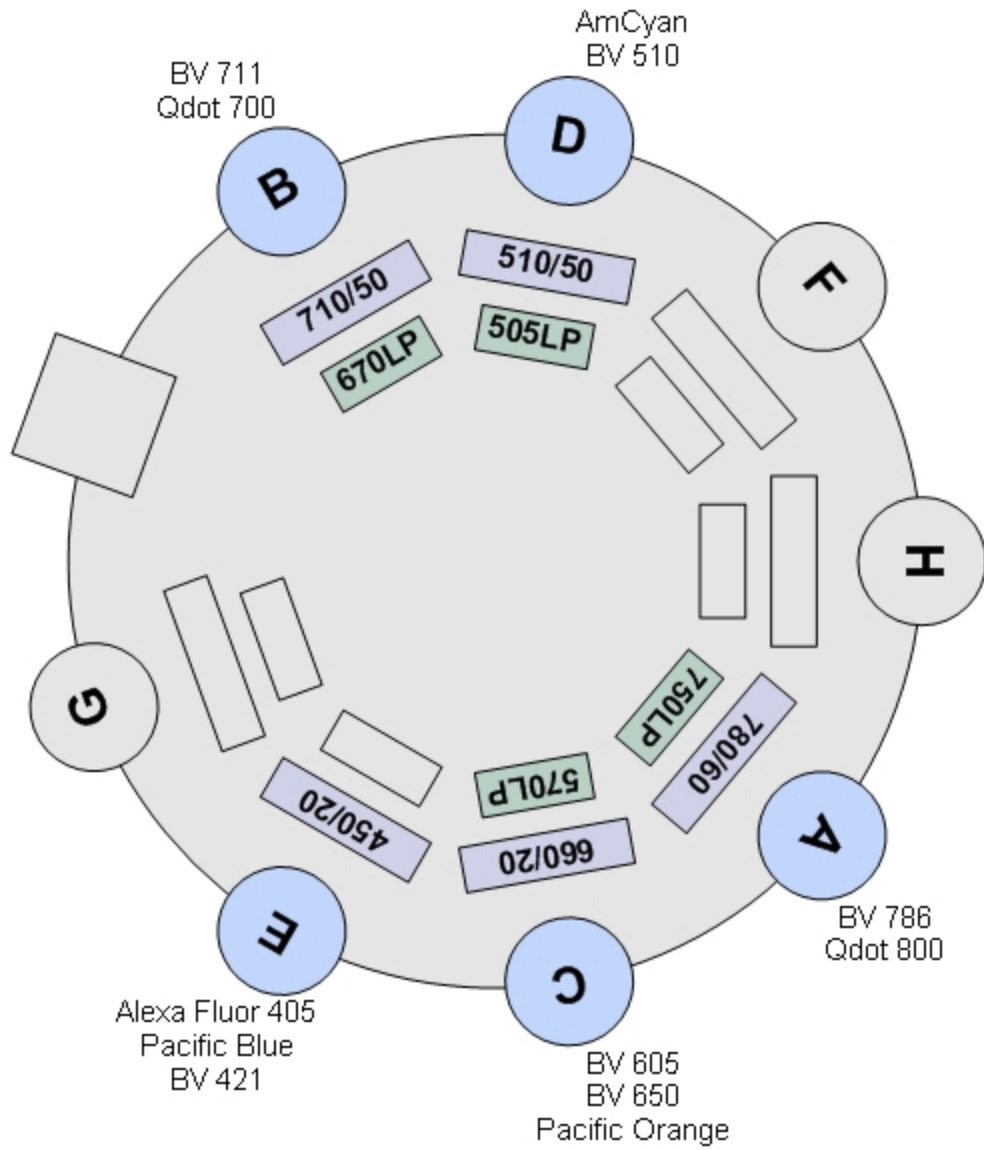

UV Laser
(355nm)

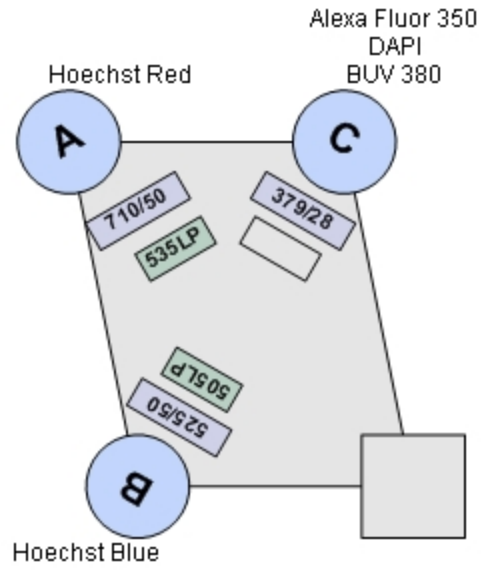

Comments: