



New SORP 4-Laser Upgrade 14-Color

Cytometer:	FACSriaII	User:	fhcrc
Cytometer Name:	FACSriaII	Institution:	
Serial Number:	1	Software:	BD FACSDiva 6.1.3
Input Device:	Manual	Date:	8/14/2017 10:44:26 AM
Sheath Pressure:	70.00		
Nozzle Size:	70		
Window Extension:	2.00		


Red Laser
(633nm)

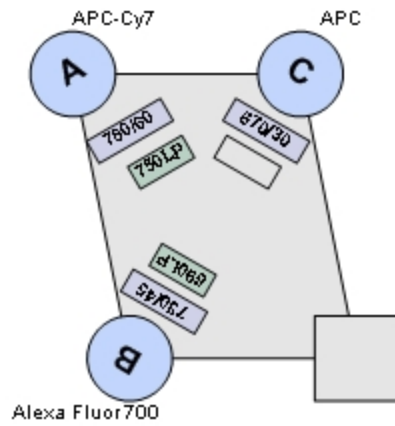


Violet Laser
(405nm)

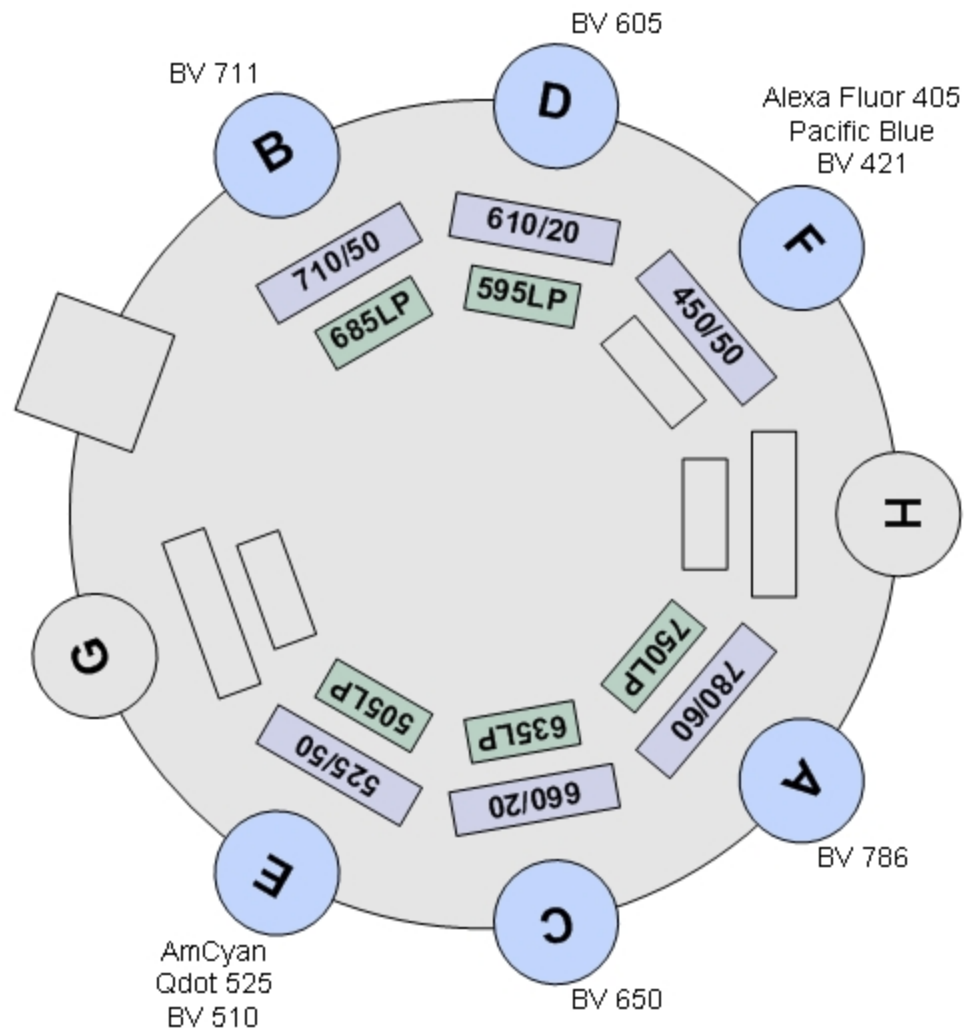

Green Laser
(552nm)

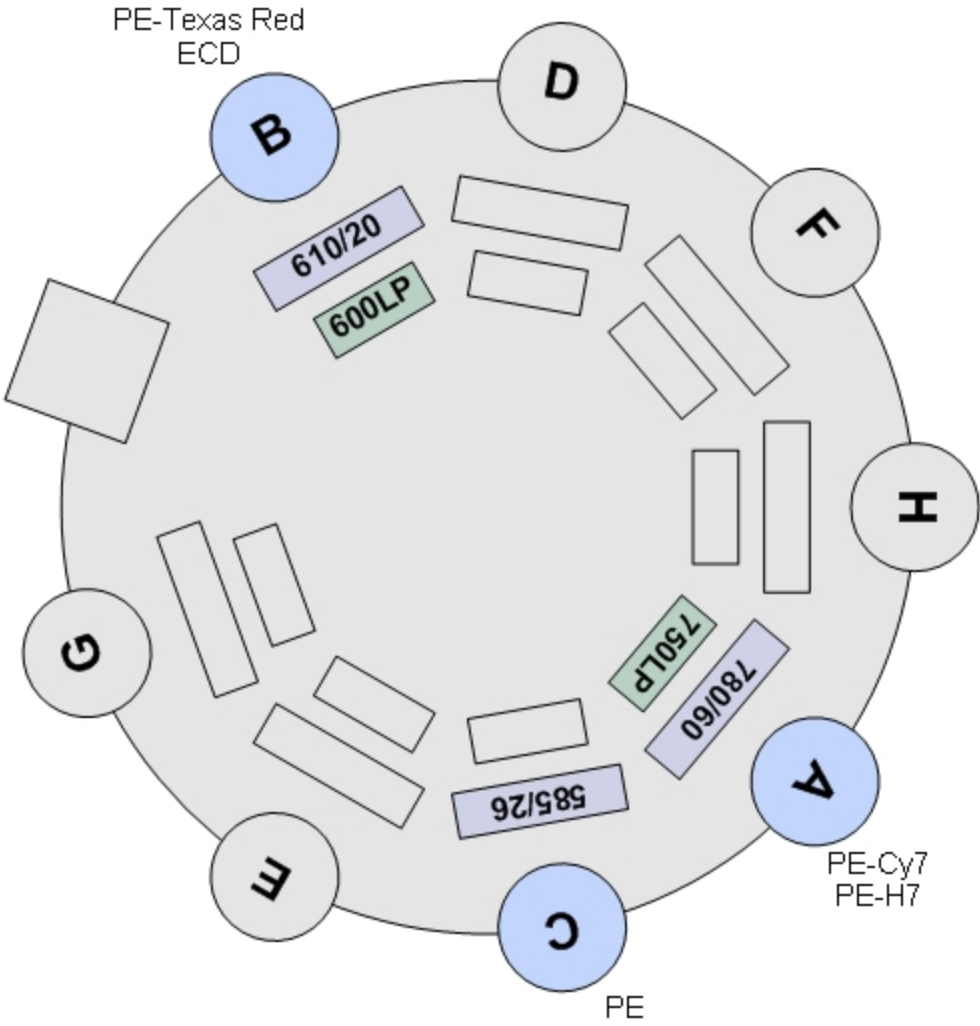

Blue Laser
(488nm)
SSC

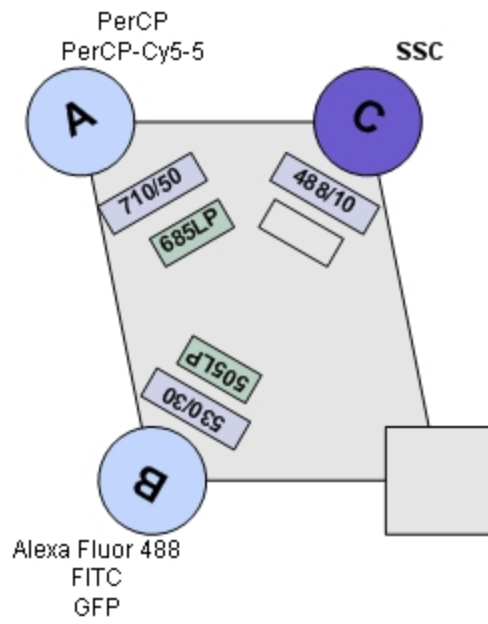

Comments: