



CST_3-laser, 8-color (4B50-2R75-2V30)

Cytometer:	FACSCantoII	User:	FHCRC
Cytometer Name:	FACSCantoII	Institution:	
Serial Number:	V33896301442	Software:	BD FACSDiva 6.1.2
Input Device:	HTS	Date:	3/23/2017 2:45:50 PM
Window Extension:	7.00		


Blue Laser
(488nm)
FSC

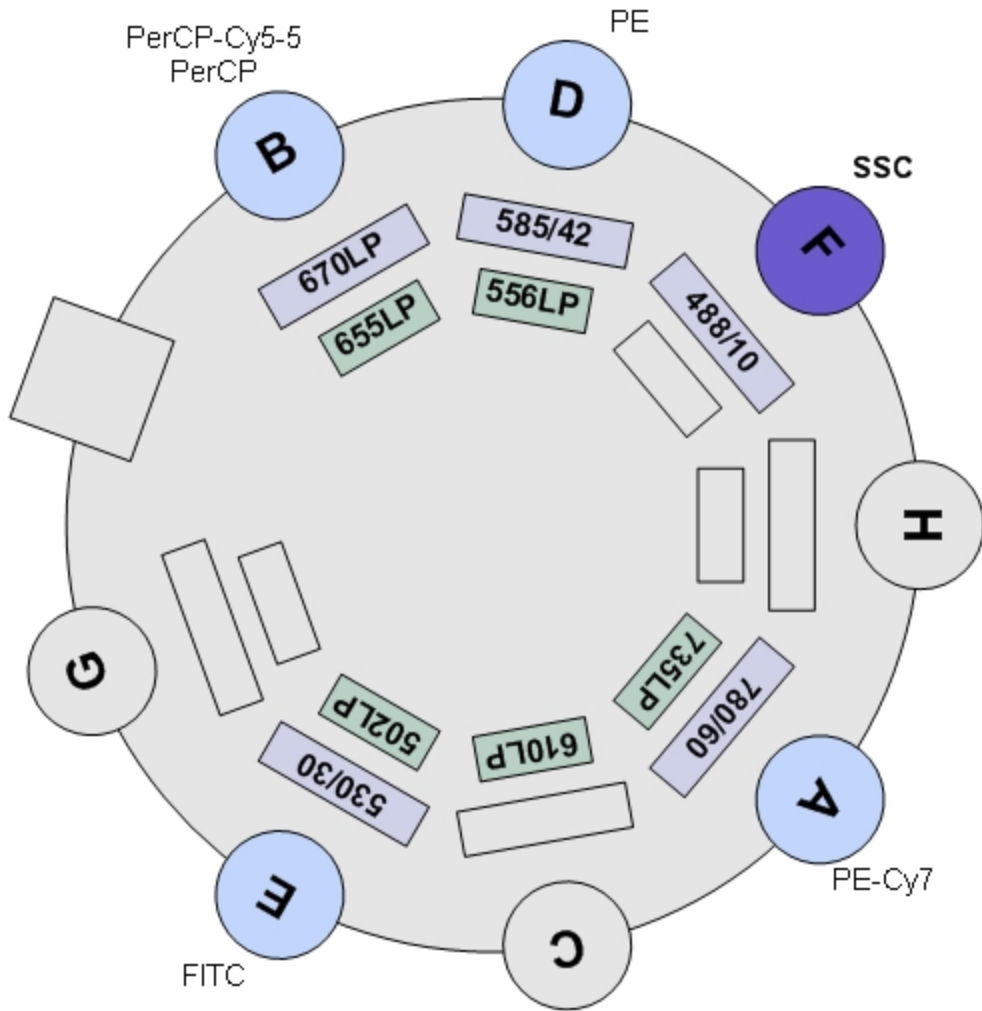

Red Laser
(633nm)

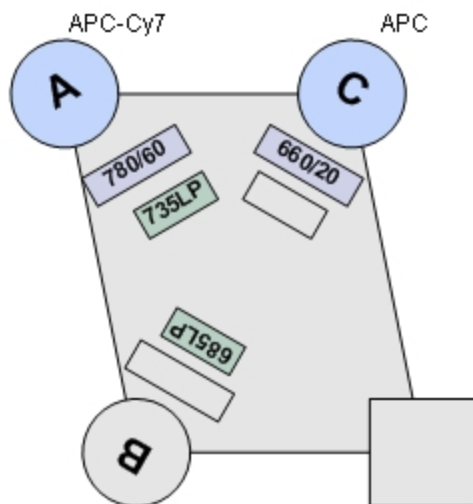

Violet Laser
(405nm)

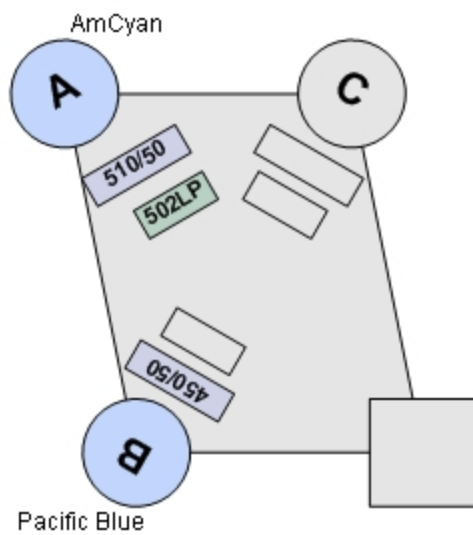

Comments: