



New Config X-50_6B-3R-5G-8V-7UV

Cytometer:	LSRFortessa	User:	FHCRC
Cytometer Name:	LSRFortessa	Institution:	N/A
Serial Number:	1	Software:	BD FACSDiva 8.0.1
Input Device:	HTS	Date:	3/23/2017 2:52:27 PM
Window Extension:	10.00		


**Blue Laser
(488nm)
FSC**

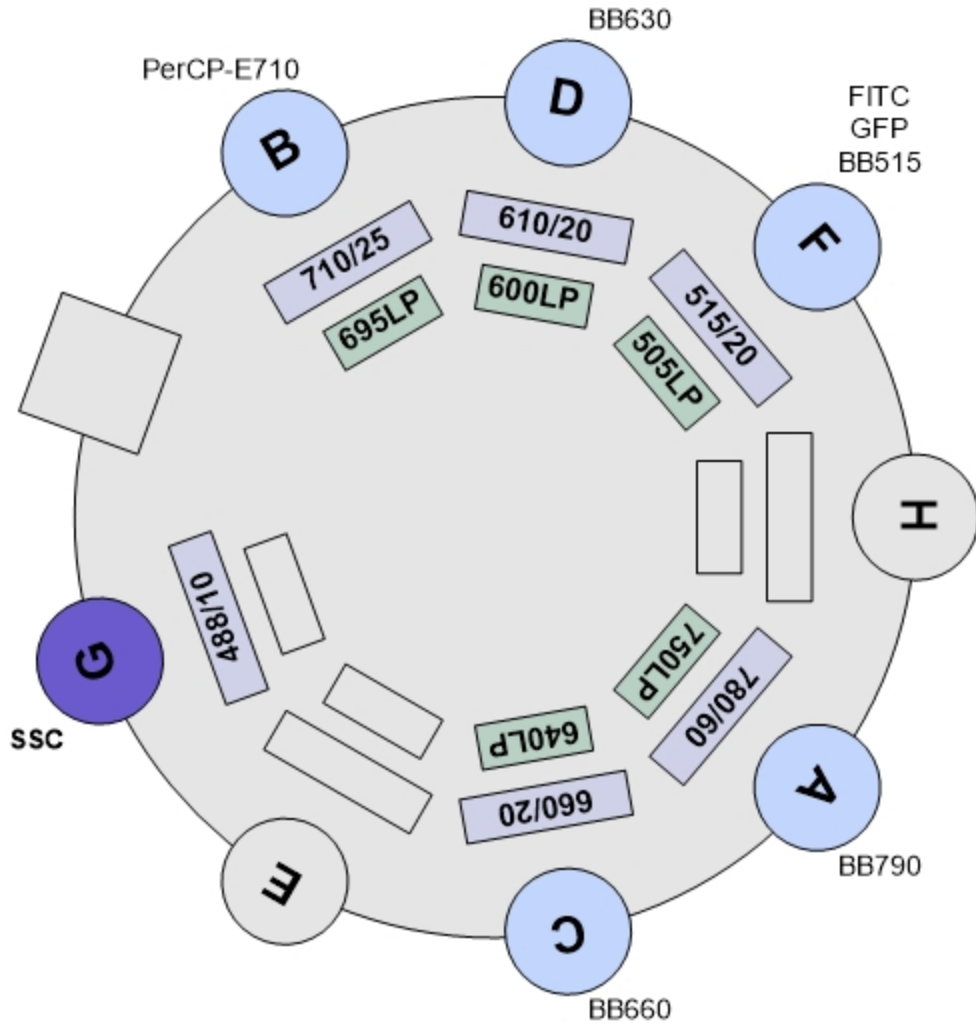


Red Laser
(628nm)

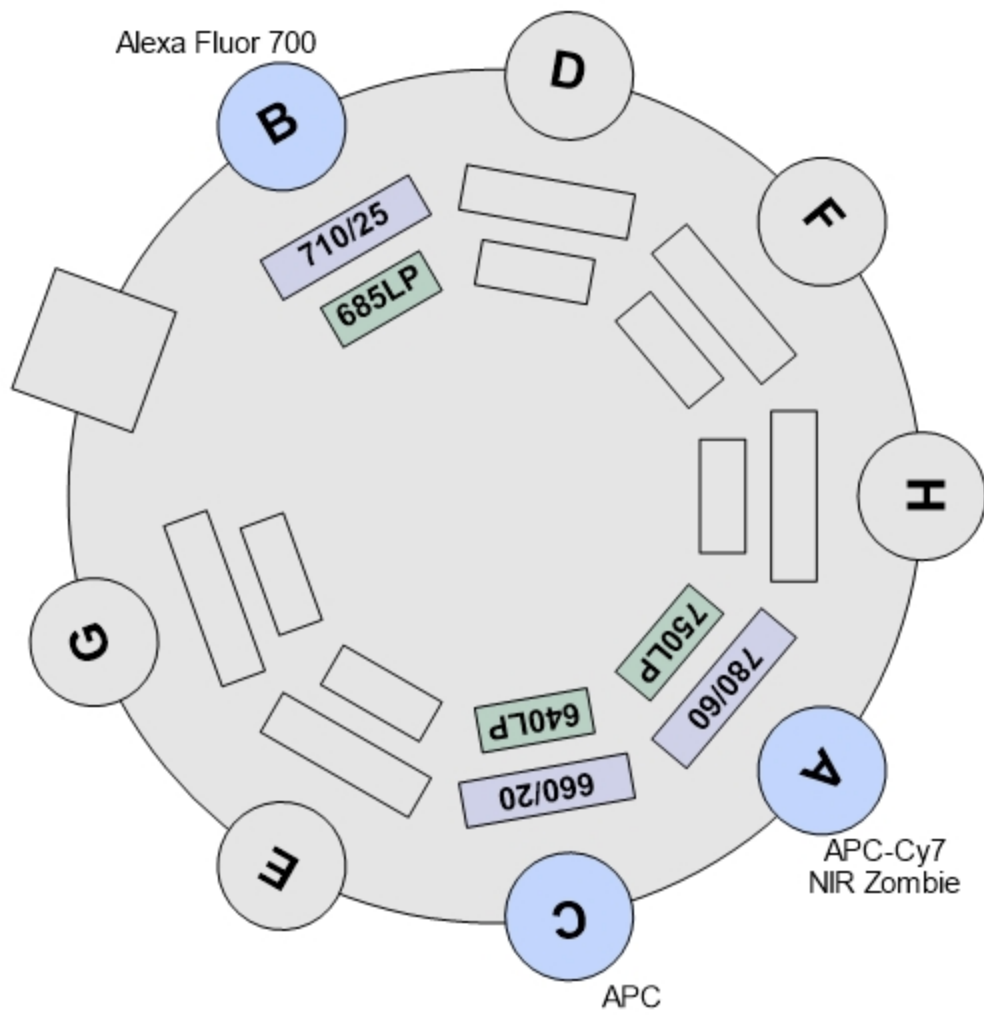


Green Laser
(552nm)

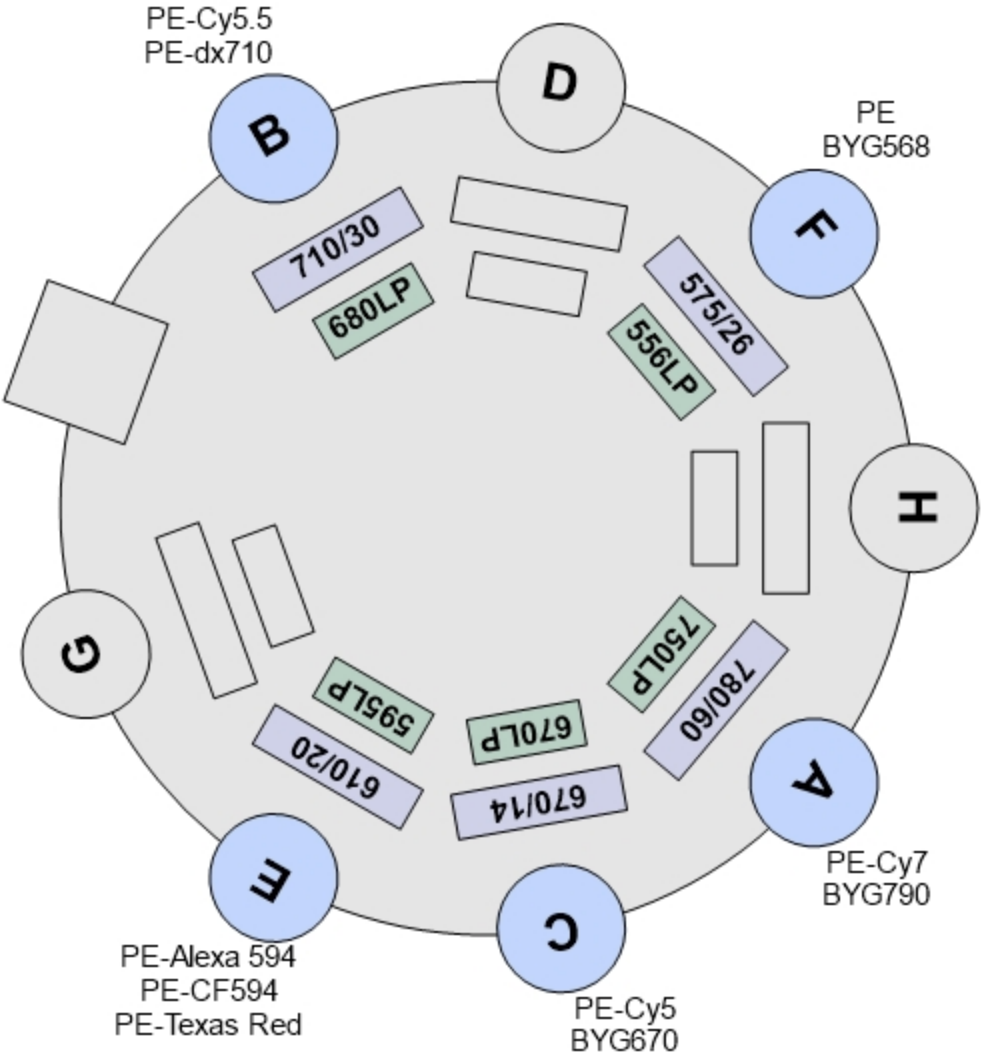


Yel-Grn Laser
(561nm)

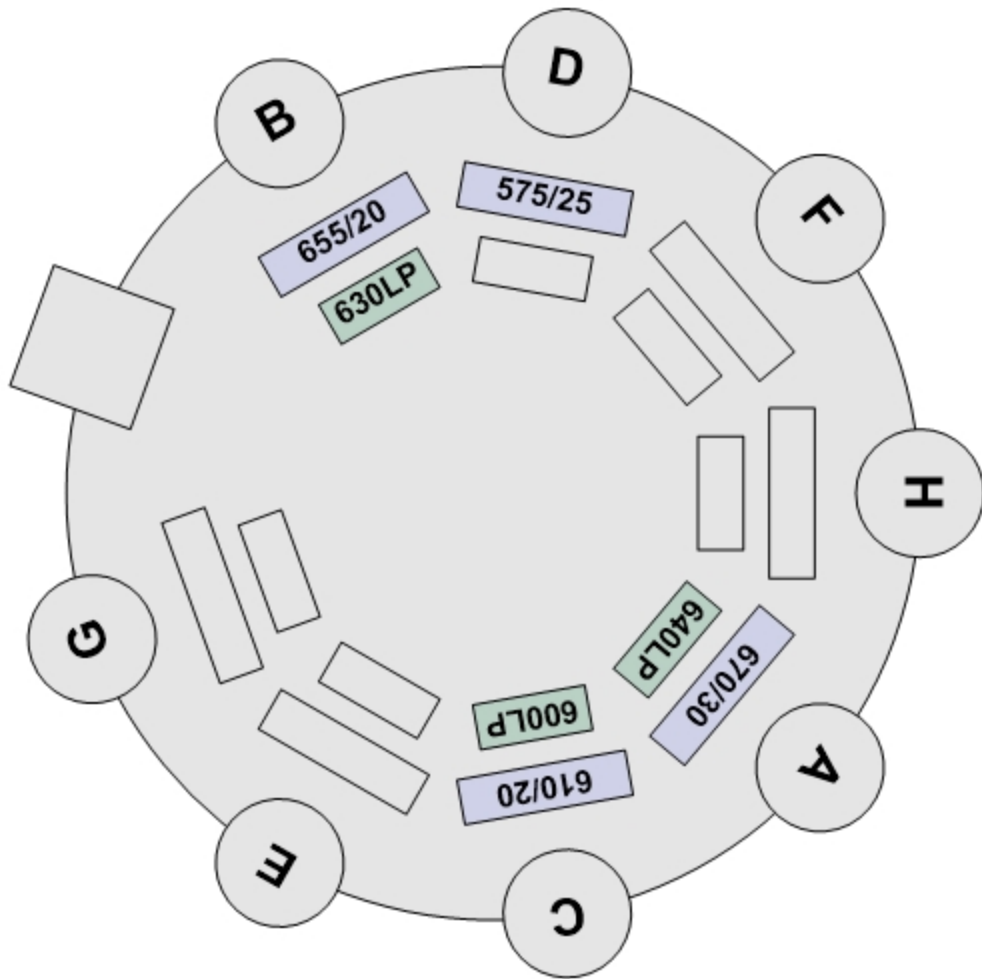

Violet1 Laser
(405nm)

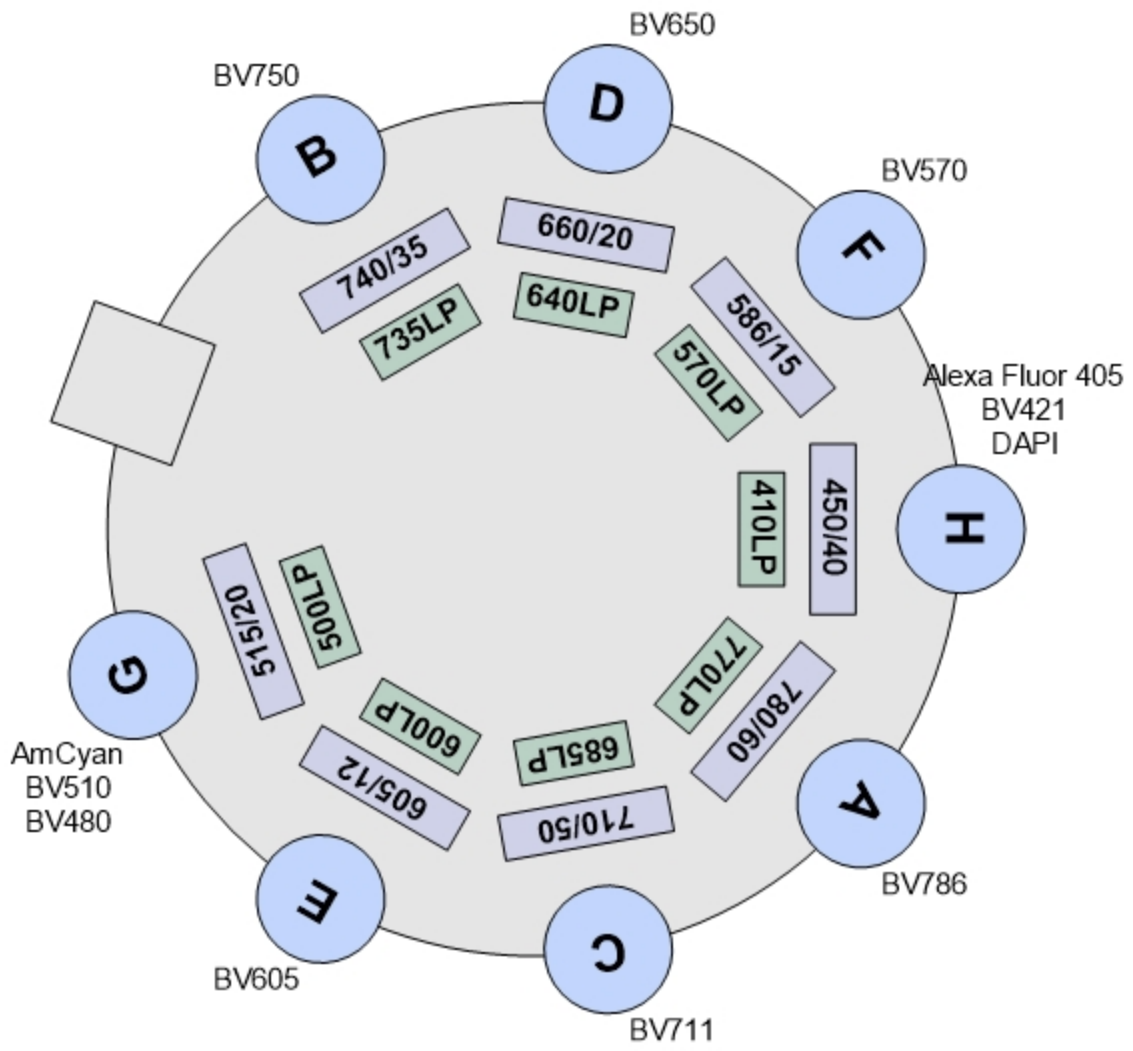

UV Laser
(355nm)

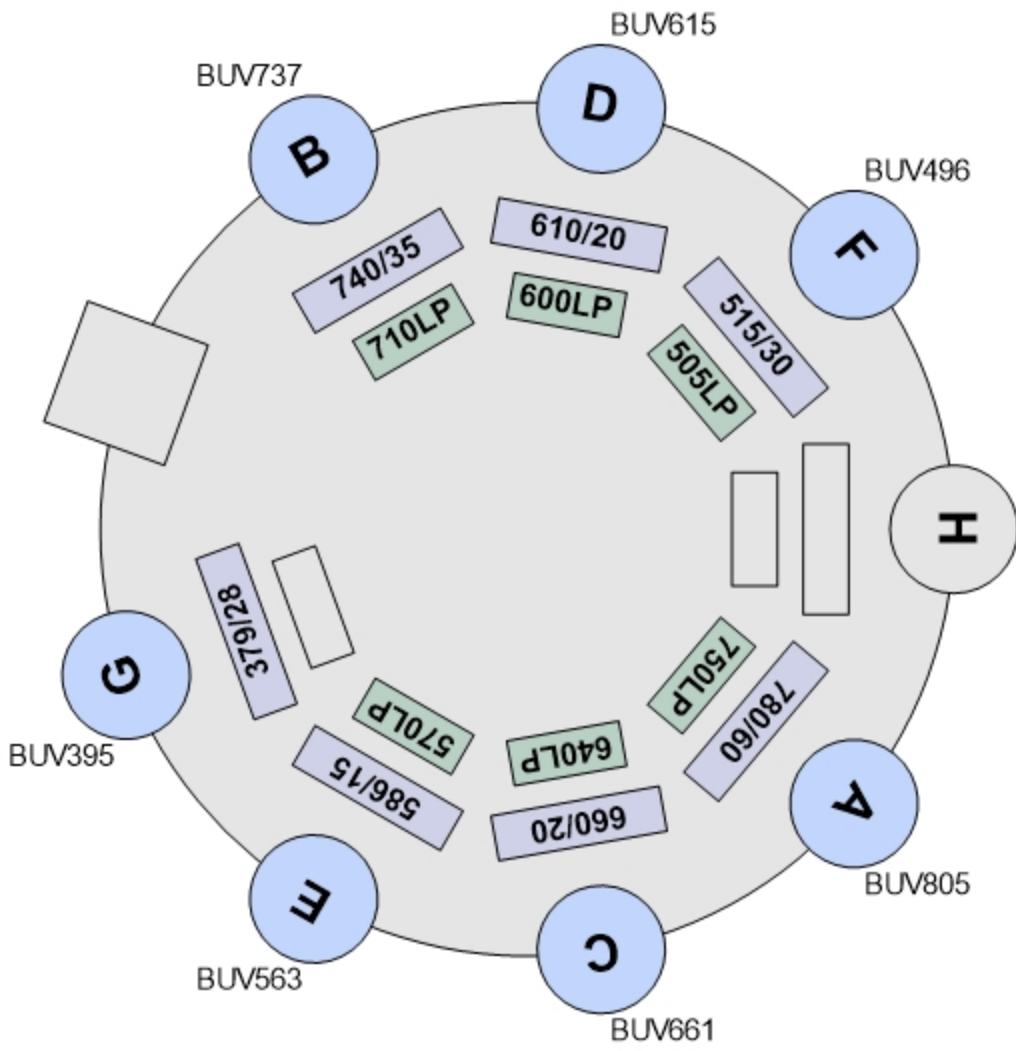

Comments: